



## 牛乳中のアフラトキシンM1の分析 Analysis of aflatoxin M1 in milk



D150721B

### Procedure




Aflatoxin M1


YMC-Triart C18 (5 μm, 250 X 4.6 mmI.D.)  
Injection : 100 μL

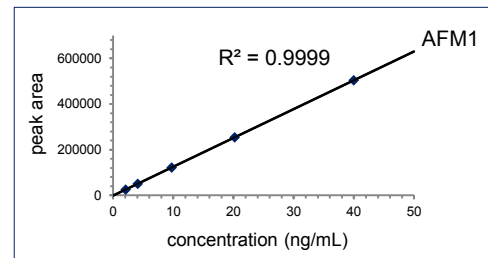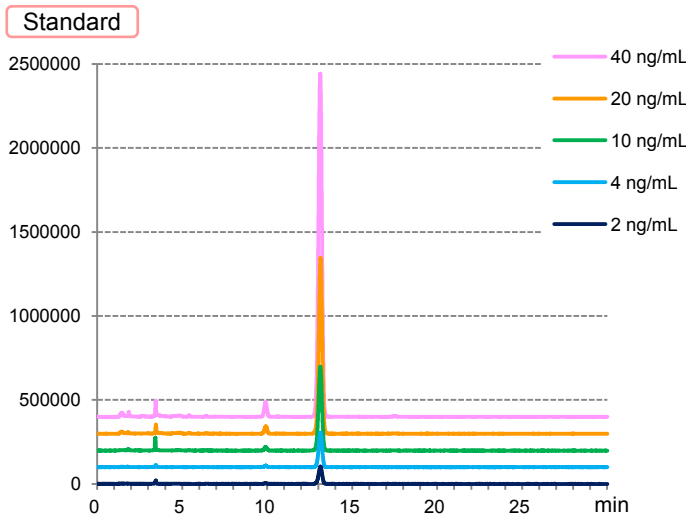


Matrix standard (10 ng/mL)

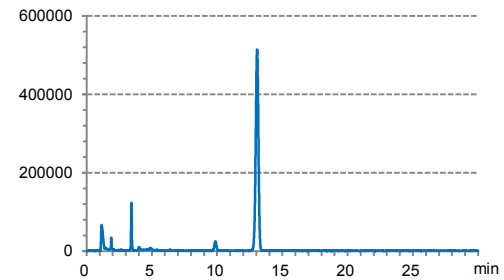

YMC-Triart C18 (5 μm, 250 X 4.6 mmI.D.)

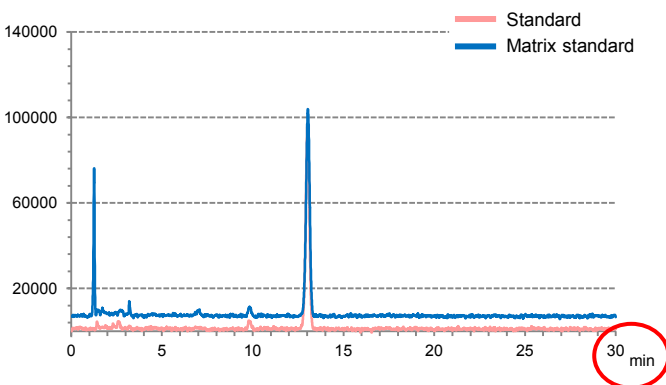

YMC-Triart C18 (3 μm, 100 X 3.0 mmI.D.)

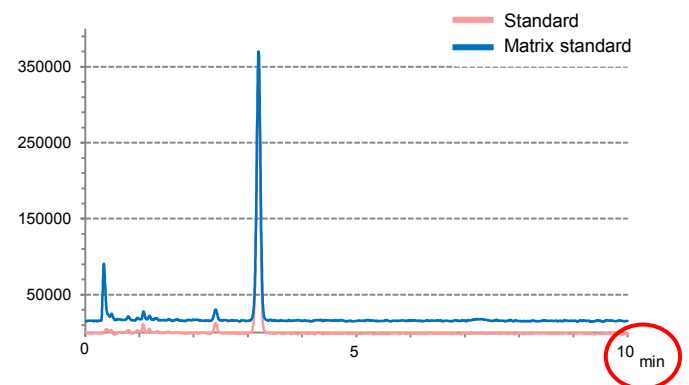

Courtesy of Japan Frozen Foods Inspection Corporation

Column : YMC-Triart C18 (12 nm)  
 Eluent : acetonitrile/water (25/75)  
 Flow rate : 1.0 mL/min for 4.6 mmI.D., 0.8 mL/min for 3.0 mmI.D.  
 Temperature : 40°C  
 Detection : FLS at Ex 365 nm, Em 435 nm  
 Injection : 20 μL